

Differences in External and Internal Cortical Strain with Prosthesis in the Femur

Olav Reikeras^{*1}, Gudrun T. Aarnes¹, Harald Steen¹, Per Ludvigsen¹ and Geir Sagvolden^{2,3}

¹Oslo University Hospital, University of Oslo, Rikshospitalet, NO-0027 Oslo, Norway

²National Defence Research Institute, NO-2007 Kjeller, Norway

³Light Structures AS, NO-0571 Oslo, Norway

Abstract: The contact between a femoral stem prosthesis and the internal surface of the cortical bone with the stress in the interface is of crucial importance with respect to loosening. However, there are no reports of strain patterns at this site, and the main aim of the current study was to investigate differences of internal and external cortical strain in the proximal femur after insertion of a stem prosthesis. The external cortical strain of a human cadaveric femur was measured with strain gauges before and after implantation of a stem prosthesis. By use of optical fibres embedded longitudinally in the endosteal cortex, deformations at the implant–internal cortex interface could also be measured. The main external deformation during loading of the intact femur occurred as compression of the medial cortex; both at the proximal and distal levels. The direction of the principal strain on the medial and lateral aspects was close to the longitudinal axis of the bone. After resection of the femoral neck and insertion of a stem prosthesis, the changes in external strain values were greatest medially at the proximal level, where the magnitude of deformation in compression was reduced to about half the values measured on the intact specimen. Otherwise, there were rather small changes in external principal strain. However, by comparing vertical strain in the external and internal cortex of the proximal femur, there were great differences in values and patterns at all positions. The transcortical differences in strain varied from compression on one side to distraction on the other and vice versa in some of the positions with a correlation coefficient of 0.07. Our results show that differences exist between the external and internal cortical strain when loading a stem prosthesis. Hence, strain at the internal cortex does not correspond and can not be deducted from measured strain at the external cortex.

Keywords: Deformation, femur, hip, optical fibre, prosthesis, strain.

INTRODUCTION

According to traditional hip biomechanics theory, based on mathematical models and finite element analysis, a bending moment acts on the proximal part of the femur [1-3]. This theory has been validated by *in vitro* [4] and *in vivo* strain gauge measurements [5]. Insertion of a prosthesis has been shown to alter the strain patterns of the proximal femur which may have adverse effects on the dynamic bone remodeling and the ultimate fate of the prosthesis [6, 7]. Hence, the prevailing principles for optimal design of prosthesis are to aim for an implant-bone fit that is close to the physiological strain patterns, especially at the proximal aspects of the femur. Strain patterns have regularly been evaluated at the external cortex, both of the intact femur and after insertion of prosthesis. However, the contact zone between the prosthesis and the femoral bone is on the internal surface of the cortex, and the stress in this interface is of crucial importance with respect to the event of loosening. To our knowledge, there are no reports of the strain patterns at this site. Strain gauges are not appropriate for application at the implant-internal cortex interface, but Optical Bragg grating fibres (OBGF) are widely used in the industry for measurements of strain. Fibre Bragg gratings are

diffracting elements printed in the core of an optical fibre. They behave like selective filters which in the fibre core reflect the spectral components of a propagating packet according to the Bragg relation $\lambda = 2n\Lambda$; where λ is the wavelength, n being the core mean refractive index and Λ the spatial period of the refractive index modulation. If the Fibre Bragg Grating is strained along the fibre axis, Λ is changed. As a result, the Bragg wavelength is shifted, which is a measure of strain. Previously, we have shown that Optical Bragg grating fibers are well suited for dynamic measurements of bone strain [8]. On this basis, the present study was undertaken to evaluate the strain patterns at the internal and external cortex of the proximal femur before and after insertion of stem prosthesis.

MATERIALS AND METHODS

One cadaveric femur was removed within 24 hours from a 64 year old male patient who died from a heart attack, packed in saline-soaked towels and stored for -80 degrees. Before testing, the specimen was thawed at room temperature, and the remaining soft tissues were removed. To fit into our testing system the condyles were removed, and the distal part of the diaphysis was cemented into a steel cylinder. The distance from the upper end of the cylinder to the tip of the greater trochanter was 180 mm.

*Address correspondence to this author at the Oslo University Hospital, University of Oslo, Rikshospitalet, NO-0027 Oslo, Norway; Tel: +47-23076013; Fax: +47 23076010; E-mail: olav.reikeras@rikshospitalet.no

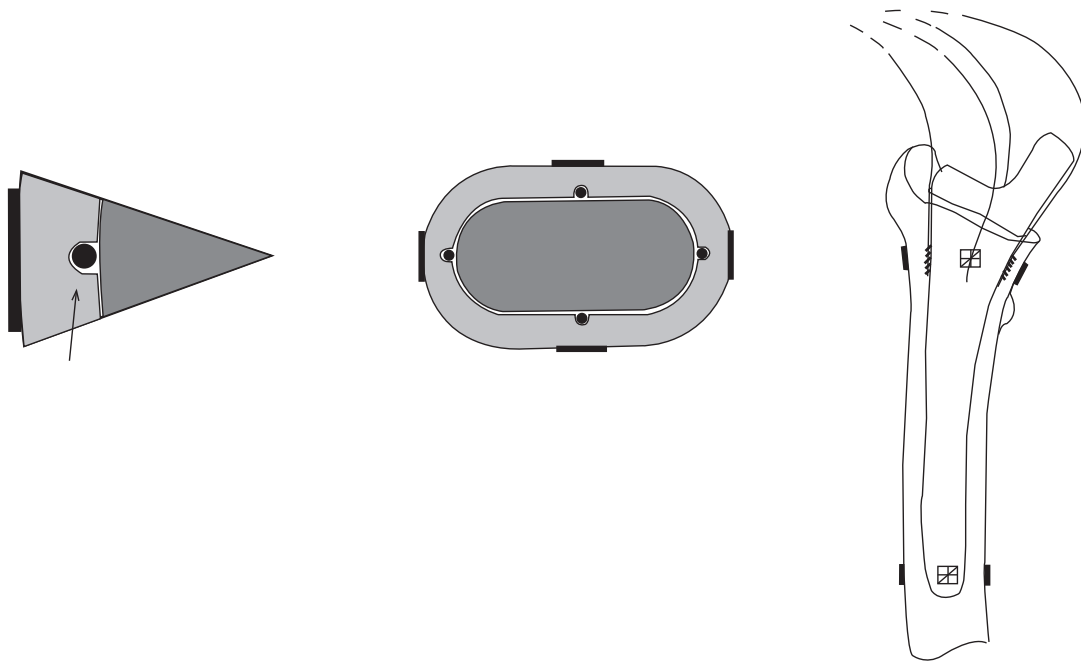


Fig. (2). Schematic drawings of the experimental set up with 4 strain gauges at the external femoral cortex both proximally and distally and 4 optical fibers at the internal femoral cortex proximally.



Fig. (3). Experimental setup with strain gauges and optical fibers (indicated by arrows). Femoral stem prosthesis cemented in the medullary canal. Loading of the specimen was performed with the femoral head component applied on the neck of the prosthesis.

RESULTS

Table 1 gives the principal external cortical strain (mean) at the proximal and distal levels of the intact femoral specimen and after neck resection and implantation of thinner and thicker titanium uncemented stem prosthesis. The main deformation during loading of the intact femur was compression of the medial cortex both at the proximal and distal level. The direction of the principal strain on the medial and lateral cortex was close to the longitudinal axis of the bone. After resection of the femoral neck and insertion of a thin uncemented prosthesis, the changes in strain values were greatest medially at the proximal level, where the deformation in compression was reduced to the half. Otherwise, there were rather small changes (less than 10% of the medial change) in principal strain. Change from the thin #9 uncemented prosthesis to a thicker #10 resulted in a 26% reduction of medial compressive strain, else the differences were less significant. Introduction of cement in the medullary canal in combination with a thin #9 prosthetic stem versus the previous uncemented #10 stem situation demonstrated a relative transfer of the compressive strain on the proximal external cortex from medial to anterior.

The external cortex (gauges) and internal cortex (fiber optical wires) vertical strain values and patterns at the proximal level with an implanted uncemented #10 and cemented #9 Titanium stem prosthesis are given in Table 2. It can be seen that also for the internal cortex optical fiber measurements, as well as for the external cortex, the strain patterns change from the uncemented to the cemented setting of the prosthesis. However, in both settings, there are great differences in strains in all positions from the external to the internal cortex of the proximal femur. The differences in strain varied from compression on one side of the bone to distraction on the other and vice versa in some of the

Table 1. Principal Strains (Microstrain), Measured by Rosette Strain Gauges at the External Cortex, at the Proximal and Distal Levels of the Femoral Specimen. Orientation Angle of the Principal Strain is Positive Counterclockwise and Relative to the Horizontal Triplet of the Rosette Gauge

		Intact Bone	Uncemented #9 Prosthesis	Uncemented #10 Prosthesis	Cemented #9 Prosthesis
Proximal	Strain (orientation)				
Medial	Maximum	496 (28°)	-82 (179°)	-45 (172°)	-32 (175°)
	Minimum	-1096 (118°)	-428 (89°)	-317 (82°)	-384 (85°)
Anterior	Max	-13 (64°)	208 (29°)	124 (28°)	73 (10°)
	Min	-147 (154°)	-196 (119°)	-161 (118°)	-269 (100°)
Lateral	Max	54 (102°)	49 (103°)	59 (106°)	59 (102°)
	Min	-32 (12°)	-31 (13°)	-41 (16°)	-38 (12°)
Posterior	Max	196 (126°)	190 (126°)	153 (124°)	190 (129°)
	Min	-151 (36°)	-141 (36°)	-123 (34°)	-195 (39°)
Distal					
Medial	Max	115 (178°)	130 (177°)	132 (176°)	126 (177°)
	Min	-491 (88°)	-501 (87°)	-477 (86°)	-466 (87°)
Anterior	Max	83 (163°)	78 (164°)	71 (166°)	103 (164°)
	Min	-183 (73°)	-230 (74°)	-196 (76°)	-230 (74°)
Lateral	Max	201 (94°)	176 (95°)	214 (97°)	172 (96°)
	Min	-76 (4°)	-29 (5°)	-34 (7°)	-64 (6°)
Posterior	Max	62 (44°)	50 (75°)	20 (89°)	89 (61°)
	Min	-79 (134°)	-32 (165°)	-36 (179°)	-55 (151°)

positions with a correlation coefficient of 0.07 for measurements.

DISCUSSION

The gold standard of measuring bone deformation under load is by application of the strain gauge, a device whose electrical resistance varies in proportion to the amount of strain. However, the use of strain gauges in humans are limited, mostly because they are difficult to adhere to bone, and the strain gauge itself and the measurement wires represent a substantial contaminant. In addition to strain gauges on the external cortex we used in the present study OBGF to measure internal cortical strain in the proximal femur after insertion of a stem prosthesis. A functional optical sensor system is a combination of a light source, sensors and an analyzer that receives the optical signals from the sensors and converts them to a format suited for digital signal processing. We found that external cortical deformation when loading is influenced by the size of the stem whether it is cemented or not, and that external cortical strain is different from internal.

A limitation of our experiment is that we have used only one human specimen and there is great variability of mechanical properties of the proximal femoral bone. However, it was not our aim to investigate such variability, but merely to investigate principal differences between strain measure on the outer cortical region as compared to the inner cortical region of the proximal femoral bone, without and with a stem prosthesis. Principally, this can be verified by one femoral specimen.

A structure monitoring system using fiber-optic sensors is based on OBGFs. The gratings are short sections of optical fiber that have been sensitized to strain and temperature through a periodic modulation of the refractive index of the fiber core. A grating reflects a narrow range of wavelengths (colours) determined by the period of the modulation. The most strongly reflected wavelength is called the Bragg wavelength and is a characteristic of the grating. The period of the grating is commonly chosen such that the reflected wavelength falls in the parts of the infrared spectrum used by the telecommunications industry, i.e. around 1300 or 1550 nm. Tensile or compressive strain on the fiber or a change in

temperature will modify the modulation period and hence the reflected wavelength. The fiber-optic sensors have a number of advantages over the electrical alternatives including a high sensitivity. Polymer coating provides good resistance toward water and chemicals, in addition to mechanical protection.

Table 2. Longitudinal (Vertical) Strain Values at the Proximal Level During Loading of 1000 N. Measured Values are from the External Cortex (Rosette Strain Gauges) and at the Internal Cortex (Fiberoptical Wires) After Implantation of an Uncemented and Cemented Titanium Prosthesis, Respectively. Negative Strain Values Designate Compression

	Uncemented #10 Prosthesis Microstrain	Cemented #9 Prosthesis Microstrain	Change with Cement Microstrain*
Medial			
External cortex	- 570	- 382	188
Internal cortex	0	- 55	- 55
Anterior			
External cortex	- 110	- 260	- 150
Internal cortex	210	203	- 7
Lateral			
External cortex	27	55	28
Internal cortex	- 90	115	205
Posterior			
External cortex	- 87	36	123
Internal cortex	- 56	135	191

* Correlation coefficient: 0.07.

When the femoral neck is cut for insertion of a prosthesis, the biomechanical function of the bone in the proximal femur is severely affected [6, 7]. The common design rationale for femoral stems is to achieve a close fit of the prosthesis to the bone to restore the strain in the proximal femur and to obtain maximum mechanical stability of the implant to minimize micromotion between the implant and the surrounding bone [9, 10]. The mechanical stability is determined by the frictional forces at the implant-endosteal bone interface, the interlocking between the implant and the bone and the elastic deformation of the bone and the implant at their interface. Alterations of the physiological strain patterns induce dynamic bone remodeling which may cause changes in bone density and geometry, and ultimately an unstable situation at the implant-bone interface will occur [7].

It has been a common opinion that stem size and stiffness are the dominant features controlling bone remodeling after hip replacement [1, 11, 12]. However, when titanium implants are compared to stainless steel with identical design, there are small differences in proximal stress shielding [6,13]. We also found some slight differences in strain patterns between a smaller and a larger stem, but it should be emphasized that the stem difference from #9 to #10 was rather small. In addition cementing of a #9 prosthesis with a cement mantle of only 1 mm does not

reflect the clinical situation. However, this was done to show the immediate effect of changing an intimate contact between the bone and the surface of the prosthesis to an interface between bone and cement surrounding the prosthetic stem. Our results are in accordance with the opinion that factors contributing to femoral cortical strains are rather complex, and that size and stiffness are less important than conformity with metal implants which are rather stiff as compared to bone [14-16].

After insertion of the implant, strain patterns are unpredictable [13, 17]. Much work has been done to obtain a design of the stem that maintains physiological strain after insertion of the implant [5, 18-20]. Strain gauge measurements usually have been employed to study the pattern of load transfer from the stem to the femur after insertion of a prosthesis. However, on the femur only external surface strain has been presented and often as longitudinal strain only.

Our aim was to measure the strain at the interface between the implant and the internal cortical bone. The strain measurements in this study showed that the strain patterns were significantly different at the internal and external cortex.

Studies of acute changes in the strain pattern in cadaver femurs after insertion of femoral stems are valuable in the assessment of implant variables. Our findings correspond to the results reported by other authors [5, 18, 19]. However, strain studies on the external cortex have been used uncritically to predict the *in vivo* performance, as the stress at the internal interface between the implant and endosteal bone never has been studied. Furthermore, deformation measurements on the external cortex have been assumed to reflect the simultaneous strain at the internal cortex. However, according to finite element analysis [20], there is a shift in stress from periosteal to endosteal surfaces when bone is put under stress. The results of the present study demonstrate that the external cortical condition does not correspond to the situation at the internal cortex. As the internal cortical surface is of utmost importance for the ingrowth of bone and stability of the prosthesis, we urge that future studies should pay attention to this fact.

ACKNOWLEDGEMENT

None declared.

CONFLICT OF INTEREST

The authors of this article state that they do not have any conflicts of interest.

REFERENCES

- [1] Rydell N. Biomechanics of the hip. Clin Orthop Rel Res 1973; 92: 6-15.
- [2] Radin EL. Biomechanics of the human hip. Clin Orthop Rel Res 1980; 152: 28-9.
- [3] Van Buskirk WC. Elementary stress analysis of the femur and tibia. In: Bone Mechanics 1989; 43-51. Ed by SC Cowin. Boca Raton, CRC Press.
- [4] Finlay JB, Chess DG, Hardie WR, Roabeck CH, Boume RB. An evaluation of three loading configurations for the *in vitro* testing of femoral strains in total hip arthroplasty. J Orthop Res 1991; 9: 749-59.
- [5] Aamodt A, Lund-Larsen J, Eine J, Andersen E, Benum P, Schnell Husby O. Changes in proximal strain following insertion of

- uncemented standard and custom femoral stems. *J Bone Joint Surg Br* 2001; 83: 921-29.
- [6] Huiskes R, Weinans H, vanRietbergen B. The relationship between stress shielding and bone resorption around total hip stems and the effects of flexible materials. *Clin Orthop Rel Res* 1992; 274: 124-34.
- [7] Cristofolini L. A critical analysis of stress shielding evaluation of hip prostheses. *Crit Rev Biomed Eng* 1997; 25: 409-83.
- [8] Fresvig T, Ludvigsen P, Steen H, Reikerås O. Fibre optic Bragg grating sensors: an alternative method to strain gauges for measuring deformation in bone. *Med Eng Phys* 2008; 30: 104-8.
- [9] Hua J, Walkers PS. Closeness of fit of uncemented stems improves the strain distribution in the femur. *J Orthop Res* 1995; 13: 339-46.
- [10] Walker PS, Robertson DD. Design and fabrication of cementless hip stems. *Clin Orthop Rel Res* 1988; 235: 25-34.
- [11] Bobyn JD, Mortimer ES, Glasman AH, Engh CA, Miller JE, Brooks CE. Producing and avoiding stress shielding. Laboratory and clinical observations of noncemented total hip arthroplasty. *Clin Orthop Rel Res* 1992; 274: 202-12.
- [12] Sumner DR, Galante JO. Determinants of stress shielding evaluation of hip prostheses. *Crit Rev Biomed* 1997; 25: 409-83.
- [13] Otani T, Whiteside LA, White SE. Strain distribution in the proximal femur with flexible composite and metallic femoral components under axial and torsional loads. *J Biomed Mater Res* 1993; 27: 575-85.
- [14] Langhans M, Hofmann D, Ecke H, Nietert M. Der Einfluss der Formgebung des Prothesenschaftes auf die Beanspruchung des proximalen Femurs. *Unfallchirurgie* 1992; 18: 266-73.
- [15] O'Connor DO, Harris WH. The paradox of femoral stress shielding: cemented versus cementless femoral fixation. *Trans Orthop Res Soc* 1992; 295.
- [16] O'Connor DO, Harris WH, Orr TE, Sedlacek RC, Lozynsky AJ. Paradox of strain shielding revisited, experimental evaluation of strain restoration: a comparison of four femoral implants. *Trans Orthop Res Soc* 1993; 445.
- [17] Vail TP, Glisson RR, Koukoubis TD, Guilak F. The effect of hip stem material modulus on surface strain in human femora. *J Biomech* 1998; 31: 619-28.
- [18] Kim YH, Kim JS, Cho SH. Strain distribution in the proximal human femur. An *in vitro* comparison in the intact femur and after insertion of reference and experimental femoral stems. *J Bone Joint Surg Br* 2001; 83: 295-301.
- [19] Østbyhaug PO, Klaksvik J, Romundstad P, Aamodt A. An *in vitro* study of the strain distribution in human femora with anatomical and customised femoral stems. *J Bone Joint Surg Br* 2009; 91: 676-82.
- [20] Pal B, Gupta S, New AM. Influence of the change in stem length on the load transfer and bone remodeling for a cemented resurfaced femur. *J Biomech* 2010; 43: 2908-14.

Received: June 8, 2011

Revised: September 1, 2011

Accepted: September 5, 2011

© Reikeras et al.; licensee Bentham Open.

This is an open access article licensed under the terms of the Creative Commons Attribution Non-Commercial License (<http://creativecommons.org/licenses/by-nc/3.0/>) which permits unrestricted, non-commercial use, distribution and reproduction in any medium, provided the work is properly cited.